Instruction and Maintenance Manual

RADIOLOGICAL SURVEY METER

OCDM Item No. CD V-720, Model No. 3A

Manufactured 1961

THE VICTOREEN INSTRUMENT COMPANY
5806 Hough Avenue • Cleveland 3, Ohio

TABLE OF CONTENTS

SECTION 1.
PRECAUTIONS

Paragraph — Page

1.1 High Impedance Circuitry .. 3
1.2 Semi-Conductor Components 3
1.3 Chamber Window 3
1.4 Electrometer Tube 3

SECTION 2.
GENERAL DESCRIPTION

2.1 Introduction 3
2.2 Sensing Element 3
2.3 Electronic Circuitry 4
2.4 Batteries 4
2.5 Meter and Controls 4
2.6 Physical Features 4

SECTION 3.
THEORY OF OPERATION

3.1 Ionization Chamber 4
3.2 Input Circuit 5
3.3 Measuring Circuit 5
3.4 Power Supply Circuit 5

SECTION 4.
INSTALLATION

4.1 Inspection 7
4.2 Battery Installation 7
4.3 Shoulder Strap Installation 7

SECTION 5.
OPERATION

Paragraph — Page

5.1 Adjustments and Readings .. 8
Step 1. Zero Adjust 8
Step 2. Circuit Check 8
Step 3. Range Selection and Reading 8

SECTION 6.
OPERATOR'S MAINTENANCE

6.1 Battery Replacement 9
6.2 Cleaning 9

SECTION 7.
PREVENTIVE MAINTENANCE

7.1 Preventive Maintenance 9

SECTION 8.
CORRECTIVE MAINTENANCE

8.1 Calibration 10
8.2 Disassembly for Corrective Maintenance 10
8.3 Trouble Shooting 11

SECTION 9.
REPLACEABLE PARTS LISTS

9.1 Electrical Components 13
9.2 Mechanical Components 15
9.3 List of Manufacturers 16

LIST OF ILLUSTRATIONS

Figure — Description — Page

1. View of CD V-720, Showing Operating Controls 2
2. View of CD V-720, Showing Major Components 2
3. Simplified Schematic Circuit Diagram 6
4. Method of Attaching Shoulder Straps 7
5. Schematic Circuit Diagram 12

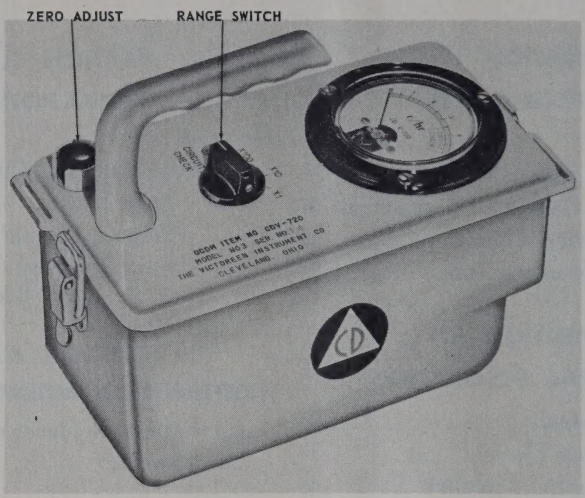

Figure 1. View of CD V-720, Showing Operating Controls

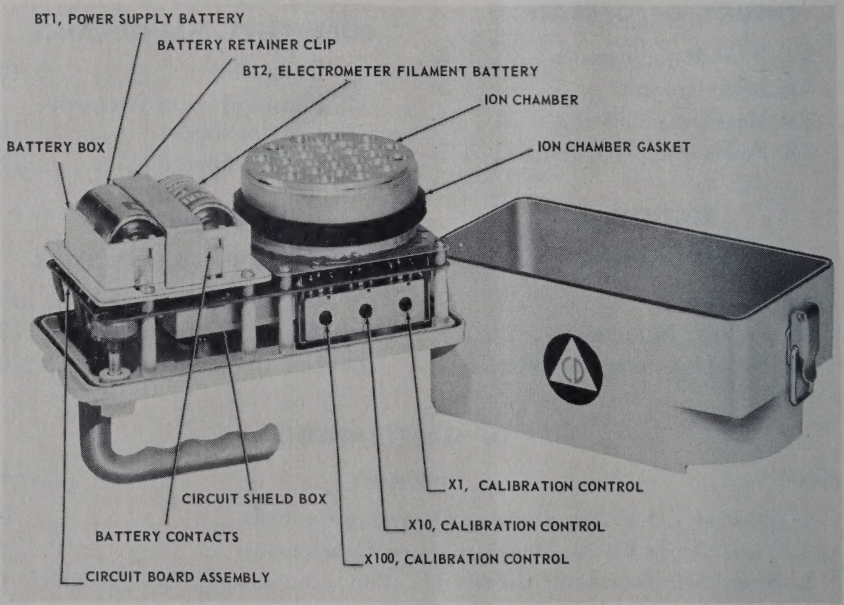

Figure 2. View of CD V-720, Showing Major Components

to the chamber electrode having the opposite charge; i.e., positive ions move toward the center electrode of the chamber and negative ions move toward the shell.
The arrival of these ions at the chamber electrode constitutes a current which is proportional to the number of ions collected. Since the number of ions created is proportional to the radiation intensity, this ionization current is proportional to the radiation intensity in the ionization chamber.

3.2 INPUT CIRCUIT:

The ionization current is extremely small—about 0.00007 microamperes at 5 r/hr which is full scale on the most sensitive range. It flows through a very high resistance (8,000 megohms) called a "Hi-Meg" connected to the collector of the ionization chamber as shown in Figure 3. This ionization current (0.00007 microamperes when the meter reads its full scale of 5 r/hr) develops a voltage drop of about 0.6 volts across the "Hi-Meg" resistor with the polarity as shown.
The voltage developed is applied to the grid of a vacuum tube for amplification. Any of the minute ionization current flowing to the grid of the tube instead of through the "Hi-Meg" resistor would result in amplification of only a portion of the signal. A special vacuum tube called an electrometer tube capable of amplifying voltages at extremely small grid currents is used to prevent this error. This tube is connected as a triode as shown in Figure 3.

3.3 MEASURING CIRCUIT:

In order to permit zeroing the instrument in a radiation field, a section of the range switch is used to short circuit the "Hi-Meg" resistor and prevent any ionization signal from being sensed by the input circuit on the "ZERO" position. A "ZERO" control is located on the top of the instrument for balancing out static plate current. This balancing is accomplished by changing the grid bias on the electrometer tube by means of the potentiometer, R7.
The measurement of the grid voltage of the electrometer tube is accomplished by metering the change in plate current directly. The static plate current is cancelled by running a reverse current, supplied by the filament battery BT2, through the meter. The magnitude of this current is fixed by the bucking resistor R9.
Sensitivity of the instrument is changed by switching "Hi-Meg" resistors, which is accomplished by the range switch.

3.4 POWER SUPPLY CIRCUIT:

Three separate d.c. voltages are required by the measuring circuit as shown in Figure 3. These are the plate voltage supply of 8 volts, the grid bias supply of —4 volts and the ion chamber collecting voltage of 50 volts.
All of these voltages are obtained from a transistor blocking oscillator circuit. The transistor Q1 permits current from BT1 to build up in the primary winding of the transformer. This current increases until the core of the specially designed transformer is saturated. When saturation is reached, the transistor is cut off by its base biasing (Sec. No. 1) and the rapid collapse in primary current (and flux) results in a voltage pulse of about 15 volts at the primary winding. This voltage pulse is rectified by CR1 and clipped or regulated at 8 volts by the zener diode CR2, to provide the current plate supply voltage.
The above regulating or clipping action carries over to the secondary

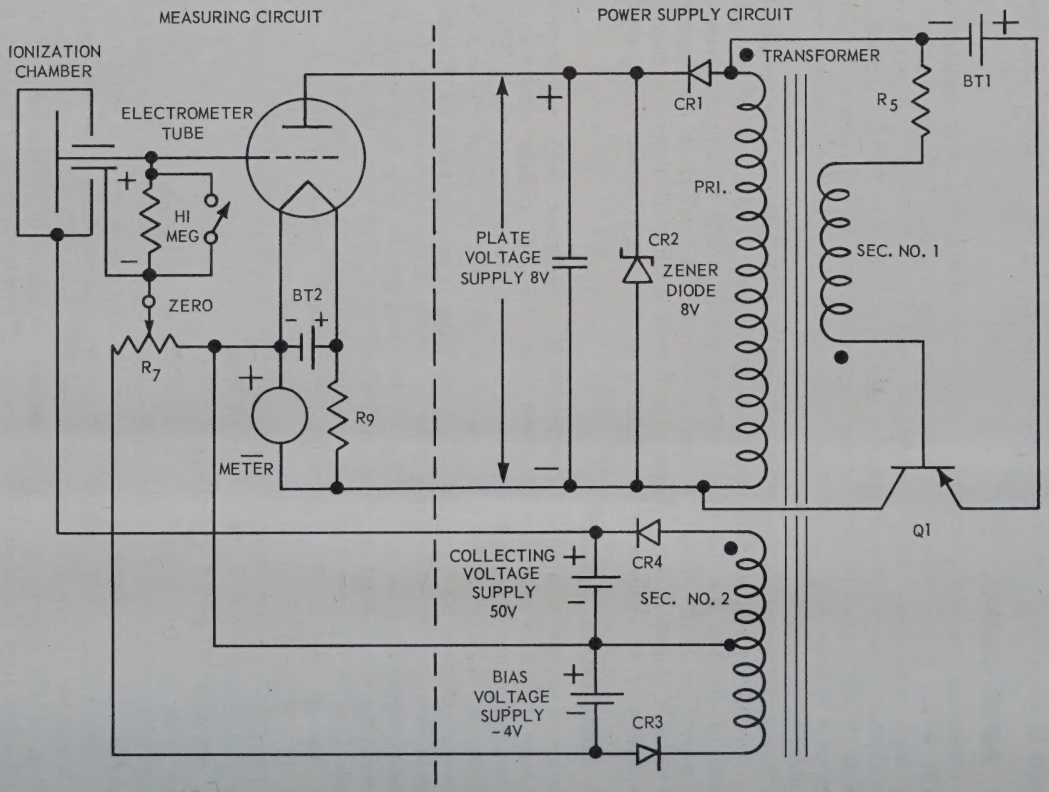

Figure 3. Simplified Schematic Circuit Diagram

to the chamber electrode having the opposite charge; i.e., positive ions move toward the center electrode of the chamber and negative ions move toward the shell.
The arrival of these ions at the chamber electrode constitutes a current which is proportional to the number of ions collected. Since the number of ions created is proportional to the radiation intensity, this ionization current is proportional to the radiation intensity in the ionization chamber.

3.2 INPUT CIRCUIT:

The ionization current is extremely small—about 0.00007 microamperes at 5 r/hr which is full scale on the most sensitive range. It flows through a very high resistance (8,000 megohms) called a "Hi-Meg" connected to the collector of the ionization chamber as shown in Figure 3. This ionization current (0.00007 microamperes when the meter reads its full scale of 5 r/hr) develops a voltage drop of about 0.6 volts across the "Hi-Meg" resistor with the polarity as shown.
The voltage developed is applied to the grid of a vacuum tube for amplification. Any of the minute ionization current flowing to the grid of the tube instead of through the "Hi-Meg" resistor would result in amplification of only a portion of the signal. A special vacuum tube called an electrometer tube capable of amplifying voltages at extremely small grid currents is used to prevent this error. This tube is connected as a triode as shown in Figure 3.

3.3 MEASURING CIRCUIT:

In order to permit zeroing the instrument in a radiation field, a section of the range switch is used to short circuit the "Hi-Meg" resistor and prevent any ionization signal from being sensed by the input circuit on the "ZERO" position. A "ZERO" control is located on the top of the instrument for balancing out static plate current. This balancing is accomplished by changing the grid bias on the electrometer tube by means of the potentiometer, R7.
The measurement of the grid voltage of the electrometer tube is accomplished by metering the change in plate current directly. The static plate current is cancelled by running a reverse current, supplied by the filament battery BT2, through the meter. The magnitude of this current is fixed by the bucking resistor R9.
Sensitivity of the instrument is changed by switching "Hi-Meg" resistors, which is accomplished by the range switch.

3.4 POWER SUPPLY CIRCUIT:

Three separate d.c. voltages are required by the measuring circuit as shown in Figure 3. These are the plate voltage supply of 8 volts, the grid bias supply of —4 volts and the ion chamber collecting voltage of 50 volts.
All of these voltages are obtained from a transistor blocking oscillator circuit. The transistor Q1 permits current from BT1 to build up in the primary winding of the transformer. This current increases until the core of the specially designed transformer is saturated. When saturation is reached, the transistor is cut off by its base biasing (Sec. No. 1) and the rapid collapse in primary current (and flux) results in a voltage pulse of about 15 volts at the primary winding. This voltage pulse is rectified by CR1 and clipped or regulated at 8 volts by the zener diode CR2, to provide the current plate supply voltage.
The above regulating or clipping action carries over to the secondary

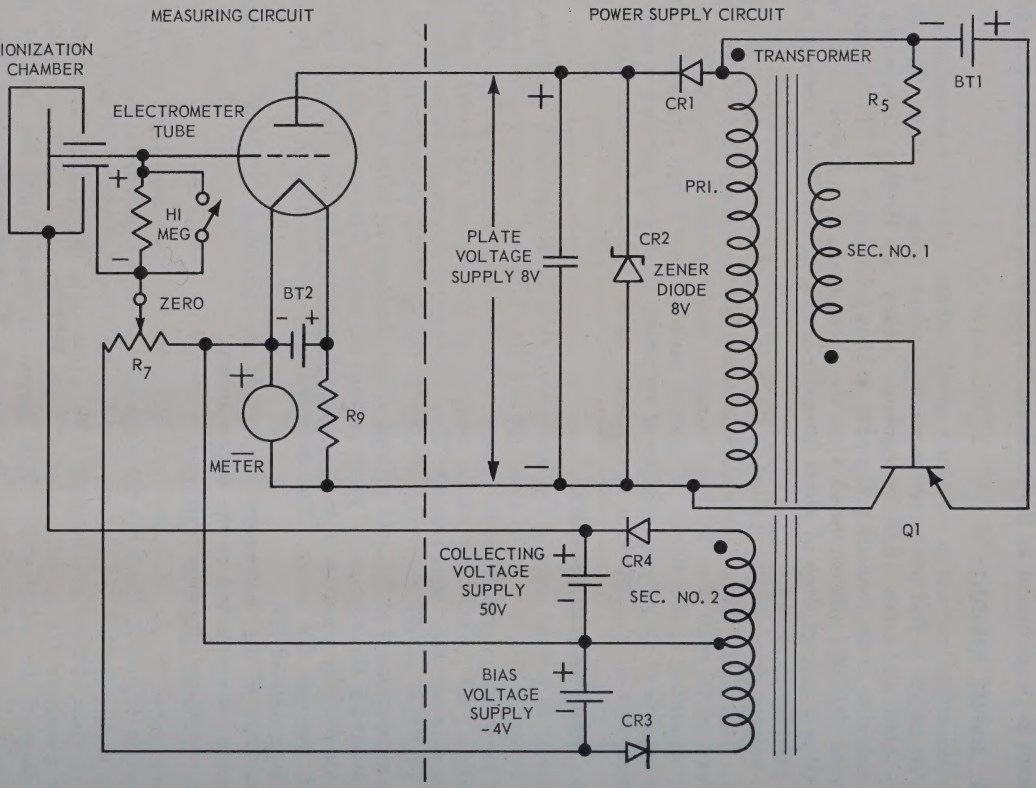

Figure 3. Simplified Schematic Circuit Diagram

winding No. 2 by reflection where the clipped voltage pulse is rectified by CR3 for the —4 volt bias supply voltage and by CR4 for the 50 volt ion chamber collecting voltage.

The oscillator circuit design with its saturating transformer utilizes the transistor as an on-off switch and assures independence of transistor parameter changes. This feature together with the zener regulator results in very low zero drift with temperature changes and battery life.

4. INSTALLATION

4.1 INSPECTION:

The instrument is shipped with batteries and carrying strap removed from the instrument and packed separately. Inspect the batteries for possible

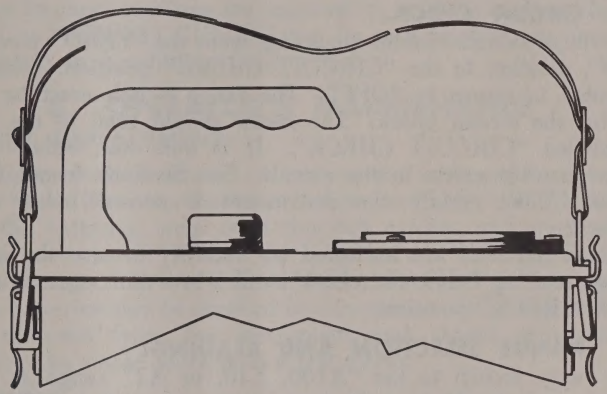

Figure 4. Method of Attaching Shoulder Straps

leakage before installation. Do not install leaking batteries. Inspect the instrument for damage in shipment. If damage is apparent the batteries should not be installed, thus preventing further damage due to possible short circuits.

4.2 BATTERY INSTALLATION:

Open the instrument by snapping open the pull catch at each end of the case and separating the top from the case bottom. This exposes the battery box and battery retainer clip as shown in Figure 2. Remove the retainer clip by squeezing its ends until it can be pulled out of the slots in the battery box. Insert the batteries in the battery box observing the indicated polarity. (The battery box is designed to be mechanically selective so that the batteries cannot be inserted with reversed polarity). Replace the battery retainer clip. Close the case by sliding the ion chamber back into its well. Align the top with the case bottom and squeeze together gently. Snap the pull catches closed.

4.3 SHOULDER STRAP INSTALLATION:

The carrying strap and two carrying strap slides and clips are packed separately. They are affixed to the cast-in carrying strap loops in the end of the case as shown in Figure 4, and the length is adjusted to suit the operator.

5. OPERATION

5.1 ADJUSTMENTS AND READINGS:

There are three simple basic steps recommended for proper operation of the CD V-720. They are described as follows:

Step 1. ZERO ADJUST.

Turn the instrument on by turning the range switch from "OFF" to the "ZERO" position. Wait about a minute to allow the electrometer tube to warm up, then orient the "ZERO" control until the meter needle indicates zero on the meter.

CAUTION

If the instrument is not zeroed properly, readings taken on any of the three ranges will be erroneous. The drift will be in an upscale direction at a very slow rate.

Step 2. CIRCUIT CHECK.

Turn the range switch counter clockwise from the "ZERO" position through the "OFF" position to the "CIRCUIT CHECK" position. This position is spring-loaded to return to "OFF". The range switch must be held in this position for the circuit check. The meter should read in the red outlined section labeled "CIRCUIT CHECK". If it does not, either the batteries are low or trouble exists in the circuit. See Sections 6 and 8 for proper procedures. Make certain the instrument is zeroed before making the circuit check.

Low or dead batteries are indicated by inability to zero the instrument or by a meter reading below the check band when the range switch is in the "CIRCUIT CHECK" position.

Step 3. RANGE SELECTION AND READING.

Turn the range switch to the "X100, X10, or X1" range as necessary to obtain an upscale reading on the meter.

The meter reading observed must be multiplied by the factor indicated by the position of the range switch to obtain the radiation dose rate in roentgens per hour (r/hr).

EXAMPLE:

METER READING	3.8
RANGE	X100
INTENSITY OF RADIATION	380 r/hr



READINGS SHOULD NOT BE TAKEN WITH POINTER INDICATING IN LOWER 10% OF SCALE (SHADED IN ILLUSTRATION). TURN TO NEXT MOST SENSITIVE RANGE UNTIL POINTER INDICATES IN UPPER 90% OF SCALE (UNSHADED).

Another example is a meter reading of 2.4 on the "X10" range which indicates a dose rate of 24 roentgens per hour while the same reading obtained with the instrument turned to the "X100" range corresponds to 240 r/hr.

A sliding beta window shutter is provided in the bottom of the instrument. This shutter has three indexed positions.

1. Completely closed—The shutter is in its most forward position and covers the beta window of the chamber.
2. 25% open—The shutter exposes 25% of the beta window to radiation from the bottom of the instrument.

3. Completely open—The shutter is in its most rearward position and exposes the complete beta window of the chamber.

For the measurement of gamma radiation dose rates only, the shutter should be in the completely closed position.

If beta radiation plus gamma radiation is to be measured, the shutter should be in the completely open or 25% open position. Under these conditions the instrument will give a reading which is the sum of the gamma and beta radiation levels. To determine the beta level alone the reading with the shutter completely closed (gamma dose rate only) should be subtracted from the reading with the shutter in an open position.

It is recommended that the beta shutter be kept closed as much as possible in order to protect the 0.006 inch thick aluminum beta window from damage. It is also recommended that the instrument be kept turned off, except for periods where frequent readings are required, in order to conserve battery life. The "ZERO" or "CIRCUIT CHECK" may be performed at any time, whether the instrument is in a radiation field or not.

6. OPERATOR'S MAINTENANCE

6.1 BATTERY REPLACEMENT:

Battery replacement is indicated whenever the instrument can no longer be zeroed or when the meter indicates below the "CIRCUIT CHECK" band. To replace the batteries, snap open the pull catches and separate the two halves of the instrument. Remove the batteries and install new batteries as indicated in Parag. 4.2 BATTERY INSTALLATION. If a voltmeter is available the batteries may be checked in accordance with Parag. 8.3. Batteries should be removed from the instrument and stored separately if the instrument is to be stored more than a few weeks.

6.2 CLEANING:

WARNING

Do not use cleaning solvents on the plastic parts. To clean the case, use soap and water. If the batteries have leaked, remove the case bottom and fill with warm water. The battery spillage will be loosened in a short while and can be rinsed out. Be careful not to soak off the circuit diagram or the CD decal.

7. PREVENTIVE MAINTENANCE

7.1 PREVENTIVE MAINTENANCE:

It is recommended that preventive maintenance procedures be carried out once a month when the instrument is in use, and about once every six months when the instrument is in storage.

Preventive Maintenance should be carried out as follows:

a. Remove the batteries, clean battery contacts and battery terminals if necessary and remove any corrosion present.
b. Replace the batteries making certain that all batteries make good contact and exceed minimum voltage.
c. Perform the operation indicated in Section 5, ZERO and CIRCUIT CHECK.

Batteries should be removed from the instrument and stored separately if the instrument is to be stored more than a few weeks.

8. CORRECTIVE MAINTENANCE

WARNING

Calibration should be attempted only by personnel trained in the use of radioactive isotope sources.

8.1 CALIBRATION:

The CD V-720 is calibrated by being placed in a gamma radiation field of known dose rate. Such fields are most commonly produced by using a radioactive material such as radium or Cobalt^{60}. As an example a 1 curie radium source will produce a radiation dose rate of 4 r/hr, at a distance of 18.1 inches. The CD V-720 should read this dose rate when so positioned with the center of the ion chamber at this distance. If it does not, the instrument should be recalibrated. This is accomplished by removing it from its case and adjusting the individual "CAL" controls for the corresponding ranges so that the proper reading is indicated on the meter. The distance from the center of the CD V-720 ionization chamber to the calibrating source should be at least 12 inches to obtain reasonable geometry (reasonably uniform radiation intensity over the volume of the ionization chamber).

If necessary to remove the instrument from its case to adjust the "CAL" controls, the instrument must be replaced in the case to obtain a correct reading.

8.2 DISASSEMBLY FOR CORRECTIVE MAINTENANCE:

a. Release the snap action catches and remove the instrument from the case bottom.

b. Remove the retaining clip and batteries from the battery box.

c. Remove the four screws which secure the battery box to the instrument top. Swing the battery box away from the circuit board. Wiring between the battery box and the circuit board prevents complete separation of the battery box.

d. Remove the four screws and spacers which secure the chamber to the instrument top.
Note: At this point the instrument (with batteries) will operate on ZERO and CIRCUIT CHECK ranges and the circuit board is completely exposed for trouble shooting.

e. Remove the meter nuts.

f. Remove the knob from the ZERO control. It is not necessary to remove the range switch knob.

g. Remove the circuit board. This is most easily accomplished by pressing on the ZERO control shaft and applying a slight pressure at the meter studs.

h. Remove the nuts, washers, and lockwashers from the top of the circuit shield box.

i. Remove the circuit shield box. The instrument is now completely disassembled.

Reassembly of the instrument is the reverse of the disassembly procedure.

CAUTION

Before beginning reassembly make certain the range switch and *both* switch wafers are oriented in the *OFF* position.

8.3 TROUBLE SHOOTING:

The majority of the electrical components of the CD V-720 are standard parts familiar to electronic technicians and are readily checked by conventional means. The electrometer tube, the "Hi-Meg" resistors, the ion chamber insulator and the ceramic switch section are the only components requiring special precaution. These components are all part of the high resistance input circuit. THE INSULATING PORTIONS OF THESE FOUR COMPONENTS SHOULD NOT BE HANDLED. They should be touched only with clean tools when repairs are made. If surface leakage on any of these items is suspected, cleaning with clean alcohol using a clean camel hair brush is recommended. Avoid solder flux splattering on these components when repairs are made.

All batteries as well as the measuring circuit are checked by the "CIRCUIT CHECK". If trouble exists, batteries should be checked with any voltmeter having a sensitivity of 1000 ohms/volt or more. The "D" cells, BT1 and BT2, should read higher than 1.2 volts.

Circuit malfunctions may be traced with the aid of the schematic circuit diagram, Figure 5. Voltage measurements shown on this diagram are measured with respect to point* and are those obtained with a voltmeter having a sensitivity of 20,000 ohms per volt. Such voltage checks should be taken with the instrument range switch turned to the "ZERO" range and with the zero control adjusted so that the instrument reads zero.

The following troubles and corrective action are presented as an aid to trouble shooting.

TROUBLE SHOOTING CHART

Trouble and Cause	*Corrective Action*
NO READING	
Filament Battery Low	Replace the Battery
Corroded Battery Contacts	Clean or Replace the Contacts
Meter Damaged	Replace Meter
Chamber Damaged	Replace Chamber
Open Connection	Inspect Solder Joints
METER WILL NOT ZERO (Reads Upscale)	
Transformer Defective	Replace Transformer
METER WILL NOT ZERO (Reads Downscale)	
Power Supply Battery Low	Replace Battery
Corroded Battery Contacts	Clean or Replace Contacts
Defective Tube	Check Tube Filament
Transformer Defective (Transformer does not "Sing")	Replace Transformer
INSTRUMENT READS LOW	
Calibration Control Disturbed	Check Calibration
Defective Tube	Replace Tube
Meter Damaged	Replace Meter
Defective Chamber	Replace Chamber
Dirty High Resistance Components	Clean High Resistance Components
INSTRUMENT READS HIGH	
Calibration Control Disturbed	Check Calibration
Damaged "Hi-Meg" Resistor	Replace "Hi-Meg" Resistor
Dirty High Resistance Components	Clean High Resistance Components

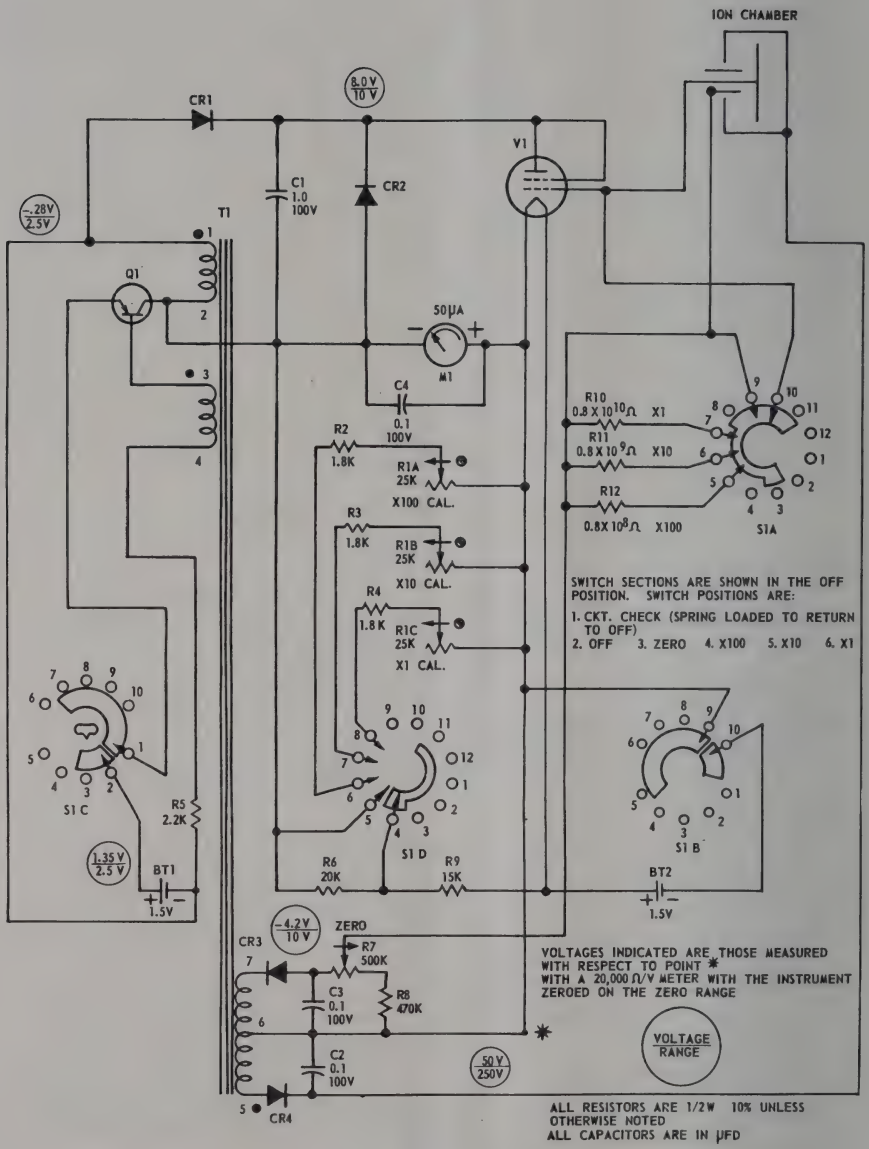

Figure 5. Schematic Circuit Diagram

8.3 TROUBLE SHOOTING:

The majority of the electrical components of the CD V-720 are standard parts familiar to electronic technicians and are readily checked by conventional means. The electrometer tube, the "Hi-Meg" resistors, the ion chamber insulator and the ceramic switch section are the only components requiring special precaution. These components are all part of the high resistance input circuit. THE INSULATING PORTIONS OF THESE FOUR COMPONENTS SHOULD NOT BE HANDLED. They should be touched only with clean tools when repairs are made. If surface leakage on any of these items is suspected, cleaning with clean alcohol using a clean camel hair brush is recommended. Avoid solder flux splattering on these components when repairs are made.

All batteries as well as the measuring circuit are checked by the "CIRCUIT CHECK". If trouble exists, batteries should be checked with any voltmeter having a sensitivity of 1000 ohms/volt or more. The "D" cells, BT1 and BT2, should read higher than 1.2 volts.

Circuit malfunctions may be traced with the aid of the schematic circuit diagram, Figure 5. Voltage measurements shown on this diagram are measured with respect to point* and are those obtained with a voltmeter having a sensitivity of 20,000 ohms per volt. Such voltage checks should be taken with the instrument range switch turned to the "ZERO" range and with the zero control adjusted so that the instrument reads zero.

The following troubles and corrective action are presented as an aid to trouble shooting.

TROUBLE SHOOTING CHART

Trouble and Cause	*Corrective Action*
NO READING	
Filament Battery Low	Replace the Battery
Corroded Battery Contacts	Clean or Replace the Contacts
Meter Damaged	Replace Meter
Chamber Damaged	Replace Chamber
Open Connection	Inspect Solder Joints
METER WILL NOT ZERO (Reads Upscale)	
Transformer Defective	Replace Transformer
METER WILL NOT ZERO (Reads Downscale)	
Power Supply Battery Low	Replace Battery
Corroded Battery Contacts	Clean or Replace Contacts
Defective Tube	Check Tube Filament
Transformer Defective (Transformer does not "Sing")	Replace Transformer
INSTRUMENT READS LOW	
Calibration Control Disturbed	Check Calibration
Defective Tube	Replace Tube
Meter Damaged	Replace Meter
Defective Chamber	Replace Chamber
Dirty High Resistance Components	Clean High Resistance Components
INSTRUMENT READS HIGH	
Calibration Control Disturbed	Check Calibration
Damaged "Hi-Meg" Resistor	Replace "Hi-Meg" Resistor
Dirty High Resistance Components	Clean High Resistance Components

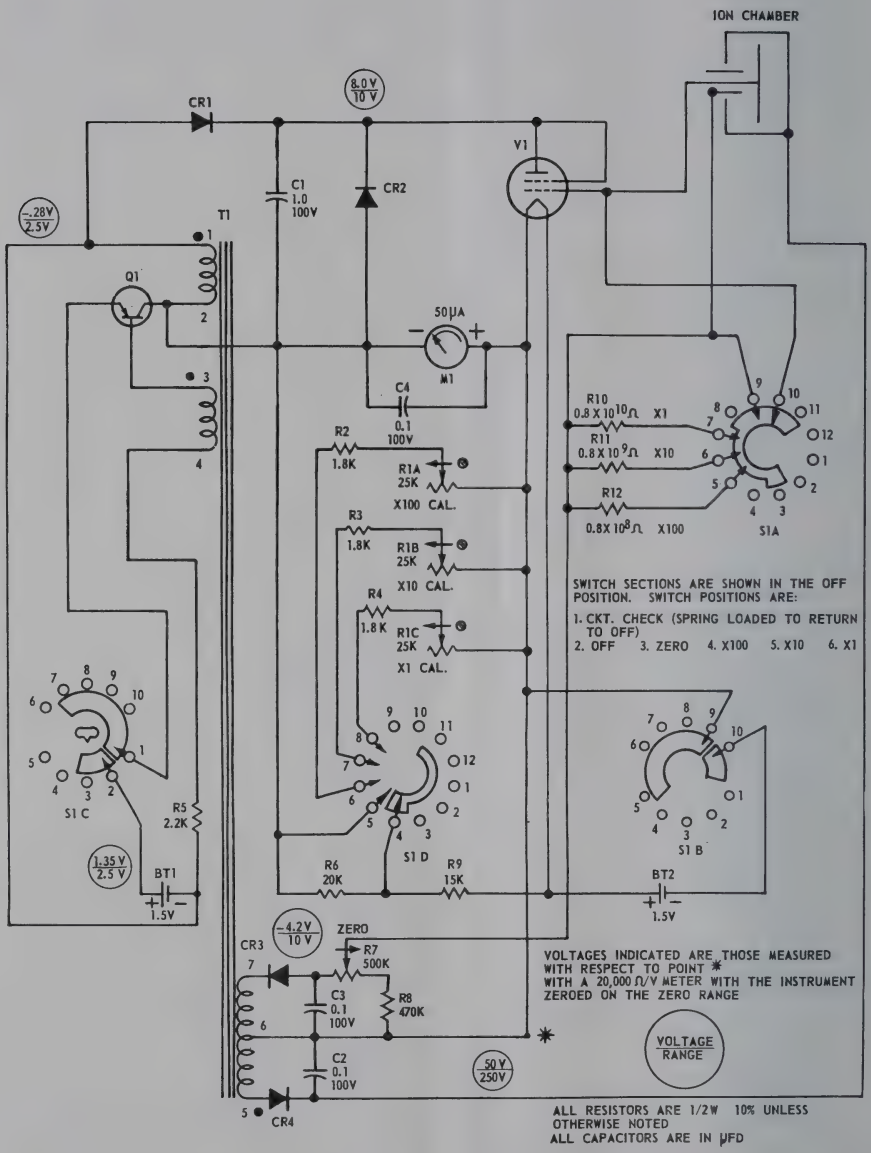

Figure 5. Schematic Circuit Diagram

9.2 Mechanical Components

Description	Function	Manufacturer	Mfg. Part No.	Victoreen Part No.	Quantity Per Equipment	*Quantity for Maintenance
Strap Buckle	Carrying Strap Length Adjustment	Waterbury Buckle Co.	807 5047	710-44	2	4
Strap Fastener	Attaches Shoulder Strap	Victoreen	700-82	700-82	2	4
Shoulder Strap	Carrying Strap	Victoreen	700-81	700-81	1	2
Case Bottom Ass'y	Bottom of Inst. Case	Victoreen	720-130	720-130	1	2
Gasket	Chamber-Case Bottom Seal	Victoreen	720-158	720-158	1	10
Knob	Zero Adjust	Harry Davies Molding Co.	1450 AC Black	720-107	1	5
Battery Retainer Clip	Holds Batteries in Box	Victoreen	720-121	720-121	1	3
Battery Contact	Elect. Connections to Batt.	Victoreen	700-68	700-68	4	15
Battery Box	Holds Batteries	Victoreen	700-66	700-66	1	3
"O" Ring Shaft Seal	Zero Adj. Shaft Seal, Switch Index	Parker Appliance Co.	5427-1	710-42	2	6
Tube Socket	Holds Electrometer Tube	Elco Mfg. Co.	805BC	720-122	1	2
Knob, Range	Selector Switch	Harry Davies Molding Co.	1500K	710-85	1	2
Meter Gasket	Cast Top-Meter Seal	Victoreen	700-63	700-63	1	5
Switch Index	Positions Range Switch	Oak Mfg. Co.	206722-J	720-106	1	3
"O" Ring	Handle—Case Top Seal	Parker Appliance Co.	2-9	46-25	1	3
Case Gasket	Case Top-Case Bottom Seal	Victoreen	720-157	720-157	1	10
Handle	Inst. Carrying Handle	Victoreen	720-114	720-114	1	3
Case Top	Top of Instrument Case	Victoreen	720-111	720-111	1	3
Instruction Manual	Operating & Maintenance Instructions	Victoreen	720-101	720-101	2	10
Spacer	Ion Chamber to Ckt. Brd. Spacer	Victoreen	720-175	720-175	4	10
Spacer	Guard Ring to Ckt. Brd. Spacer	Victoreen	720-117	720-117	1	5
Switch Drive Shaft	Connects Switch Index to Switch Wafers	Victoreen	720-126	720-126	1	3
Shield Box	Shields High Impedance Ckt.	Victoreen	720-123	720-123	1	1
Grommet	Holds Switch Drive Shaft in Shield Box	Philpott Rubber Co.	GB-225	373-75	1	1
Chamber Contact Spring	Connects Chamber Center Electrode to Elect. Tube Grid	Victoreen	720-153	720-153	1	2

*Quantity of plant and field maintenance supply parts based on five instruments for one year of operation.

9.3 List of Manufacturers

CENTRALAB DIVISION, GLOBE UNION, 900 East Keefe Avenue, Milwaukee, Wisconsin

COMPUTER DIODE CORPORATION, 250 Garibaldi Avenue, Lodi, New Jersey

CTS OF ASHVILLE, 1142 Beardsley Avenue, Elkhart, Indiana

ELCO CORPORATION, "M" Street, Philadelphia, Pennsylvania

HARRY DAVIES MOLDING COMPANY, 1428 North Wells Street, Chicago 10, Illinois

JOHN E. FAST COMPANY, 3580 North Elston Avenue, Chicago 18, Illinois

INTERNATIONAL RESISTANCE COMPANY, 401 North Broad Street, Philadelphia, Pennsylvania

OAK MANUFACTURING COMPANY, 1260 North Clybourn, Chicago, Illinois

PACIFIC SEMICONDUCTORS, INC., 10451 West Jefferson Boulevard, Culver City, California

PARKER APPLIANCE COMPANY, 17325 Euclid Avenue, Cleveland 12, Ohio

PHILPOTT RUBBER COMPANY, 2077 East 30th Street, Cleveland 15, Ohio

TUNG-SOL ELECTRIC, INC., 1 Summer Avenue, Newark, New Jersey

UNION CARBIDE CONSUMERS COMPANY., 30 East 42nd Street, New York, New York

VICTOREEN INSTRUMENT COMPANY, 5806 Hough Avenue, Cleveland 3, Ohio

WATERBURY BUCKLE COMPANY, 862 South Main Street, Waterbury 20, Connecticut